



LTP LIQUID TEMPERATURE PROBE INSTALLATION GUIDE:

1. Probe tip can be submerged into liquids with supplied adjustable compression fitting holding it in place
2. Compression fitting has an 1/8"-27 NPT Male Thread:
3. Thermocouple is Type K
4. Probe Sheath may be bent as shown below...




Correct Orientation to Bend Probe:

✔ YES




Incorrect Orientation to Bend Probe:

✘ NO



Correct Bend Radius:

✔ YE

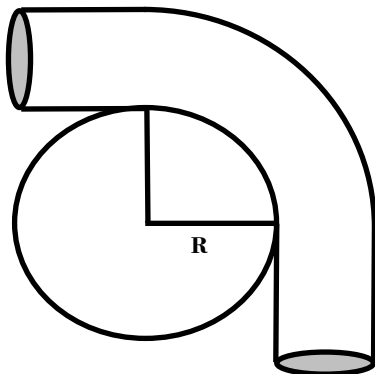

Minimum Bend Radius (R) = 3/8" (0.35")

Incorrect Bend Radius:

✘ NO

